

IOTest[®] 3
CD14-FITC /
CD16-PE /
CD45-ECD

REF A07715
 25 tests; 0.5 mL
 20 µL / test



IOTest 3
 Conjugated Antibodies



ENGLISH	Specification of constituent 1	Specification of constituent 2	Specification of constituent 3
Specificity	CD14	CD16	CD45
Clone	RMO52	3G8	J33
Hybridoma	SP2/0 x Balb/c	SP2/0 x Balb/c	NS1 x Balb/c
Immunogen	Human monocytes	Human neutrophils	Cells belonging to Laz 221 line
Immunoglobulin	IgG2a	IgG1	IgG1
Species	Mouse	Mouse	Mouse
Source	Ascites	Ascites	Ascites
Purification	Protein A affinity chromatography	Protein A affinity chromatography	Protein A affinity chromatography
Fluorochrome	Fluorescein isothiocyanate (FITC)	R Phycoerythrin (PE)	R Phycoerythrin - Texas Red [®] - X (ECD [™])
λ excitation	488 nm	488 nm	488 nm
Emission peak	525 nm	575 nm	613 nm
Buffer	PBS pH 7.2 plus 2 mg / mL BSA and 0.1% NaN ₃		

USE

This fluorochrome-conjugated antibody mixture is suitable for multiparametric analysis using flow cytometry. It permits the detection of the expression of CD14, CD16 and CD45 antigens in leucocytes.

PRINCIPLE

This test is based on the ability of specific monoclonal antibodies to bind to the antigenic determinants expressed by leucocytes. Specific staining of the leucocytes is performed by incubating the sample with the IOTest 3 reagent. The red cells are then removed by lysis and the leucocytes, which are unaffected by this process, are analyzed by flow cytometry. The flow cytometer analyzes light diffusion and the fluorescence of cells. It makes possible the localization of cells within the electronic window defined on a histogram, which correlates the orthogonal diffusion of light (Side Scatter or SS) with the fluorescence of ECD, corresponding to CD45 staining. Other histograms combining two of the different parameters available on the cytometer are also used in the gating stage. The cell population thus gated is subdivided into sub-populations, using the two other fluorescences. In this way, the positively-stained cells are distinguished from the unstained cells. The results are expressed as a percentage of fluorescent cells in relation to all the events acquired by the gating.

EXAMPLES OF CLINICAL APPLICATIONS

The CD14 antigen is found at the surface of cells belonging to the myelo-monocytic line committed to the monocytic route of differentiation. However, it is absent from B and T lymphocytes, from NK (Natural Killer) cells, from red blood cells, and from platelets (1). The CD16 antigen is the weak affinity receptor for G (IgG) immunoglobulins (FcγRIII), which is expressed on NK cells, monocytes, macrophages, and on neutrophils (2, 3). Expression of the CD45 antigen is helpful in the phenotyping of leukaemias by gating blast cells on a histogram which correlates the orthogonal diffusion of light (Side Scatter) with CD45 fluorescence. The blast cells usually express CD45 more weakly than normal cells (4, 5). This IOTest 3 reagent serves in the characterization of myeloid leukaemias. Granulocytic blast cells are identified on the basis of poor expression or CD16 negativity, whilst cells committed to the monocytic cell line are CD14⁺ (6).

STORAGE AND STABILITY

The conjugated liquid forms must be kept at between 2 and 8°C and protected from light, before and after the vial has been opened. Stability of closed vial: see expiry date on vial. Stability of opened vial: the reagent is stable for 90 days.

PRECAUTIONS

1. Do not use the reagent beyond the expiry date.
2. Do not freeze.
3. Let it come to room temperature (18 – 25°C) before use.
4. Minimize exposure to light.
5. Avoid microbial contamination of the reagents, or false results may occur.
6. Antibody solutions containing sodium azide (NaN₃) should be handled with care. Do not take internally and avoid all contact with the skin, mucosa and eyes. Moreover, in an acid medium, sodium azide can form the potentially dangerous hydrazoic acid. If it needs to be disposed of, it is recommended that the reagent be diluted in a large volume of water before pouring it into the drainage system so as to avoid the accumulation of sodium azide in metal pipes and to prevent the risk of explosion.
7. All blood samples must be considered as potentially infectious and must be handled with care (in particular: the wearing of protective gloves, gowns and goggles).
8. Never pipette by mouth and avoid all contact of the samples with the skin, mucosa and eyes.
9. Blood tubes and disposable material used for handling should be disposed of in ad hoc containers intended for incineration.

SAMPLES

Venous blood or bone marrow samples must be taken using sterile tubes containing an EDTA salt as the anticoagulant. The use of other anticoagulants is not recommended. The samples should be kept at room temperature (18 – 25°C) and not shaken. The samples should be homogenized by gentle agitation prior to taking the test sample. The samples must be analyzed within 24 hours of venipuncture.

METHODOLOGY

NECESSARY MATERIAL NOT SUPPLIED

- Sampling tubes and material necessary for sampling.
- Automatic pipettes with disposable tips for 20, 100 and 500 µL.
- Plastic haemolysis tubes.
- Calibration beads: Flow-Set[™] Fluorospheres (Ref. 6607007).

- To obtain optimal results, the following reagents are recommended:
 - Lysing reagent: IOTest 3 Lysis Solution (Ref. A07799).
 - Fixation reagent: IOTest 3 Fixative Solution (Ref. A07800).
 - One of the following IOTest 3 negative controls:
 - Neg.Ctrl.-FITC /Neg.Ctrl.-PE/CD45-ECD (Ref. A07729) or
 - Neg.Ctrl.-FITC /Neg.Ctrl.-PE/Neg.Ctrl.-ECD (Ref. A07732).
 - Buffer (PBS): 0.01 M sodium phosphate; 0.145 M sodium chloride; pH 7.2).
 - Centrifuge.
 - Automatic agitator (Vortex type).
 - Flow cytometer.

PROCEDURE

- For each sample analyzed, in addition to the test tube, one control tube is required in which the cells are mixed with the IOTest 3 negative control (Ref. A07729 or A07732).
1. Add 20 µL of specific IOTest 3 conjugated antibodies to each test tube, and 20 µL of the appropriate negative control to each control tube.
 2. Add 100 µL of the test sample to the 2 tubes. Vortex the tubes gently.
 3. Incubate for 15 to 20 minutes at room temperature (18 – 25°C), protected from light.
 4. Then perform lysis of the red cells, if necessary, by adding 2 mL of IOTest 3 Lysis Solution (Ref. A07799) at its working concentration (1X). Vortex immediately and incubate for 10 minutes at room temperature, protected from light. If the sample does not contain red cells, add 2 mL of PBS.
 5. Centrifuge for 5 minutes at 300 x g at room temperature.
 6. Remove the supernatant by aspiration.
 7. Resuspend the cell pellet using 3 mL of PBS.
 8. Repeat stage 5.
 9. Remove the supernatant by aspiration and resuspend the cell pellet using:
 - 0.5 mL or 1 mL of IOTest 3 Fixative Solution (Ref. A07800) at its working concentration (1X), if the preparations are to be kept for more than 2 hours and for less than 24 hours,
 - 0.5 mL or 1 mL of PBS without formaldehyde, if the preparations are to be analyzed within 2 hours.
- NOTE:** In all cases, keep the preparations between 2 and 8°C and protected from light

PERFORMANCE

SPECIFICITY

The RM052 monoclonal antibody (mAb) was assigned to CD14 during the 6th HLDA Workshop on Human Leucocyte Differentiation Antigens, held in Kobe, Japan, in 1996 (WS Code: MA62, Section M) (7).

MAB 3G8 was assigned to CD16 during the 4th HLDA Workshop of Vienna, Austria, in 1989 (WS Code: 409, Section NL) (8).

MAB J33 stains all the isoforms of the CD45 molecule; it is therefore referenced as a pan-leucocytic marker. MAB J33 was assigned to CD45 during the 3rd HLDA Workshop, Oxford, England, in 1986 (WS Code: 818, Section NL) (9).

LINEARITY

To test the linearity of staining for the CD14 and CD45 specificities of this reagent, a positive THP1 cell line (CD14⁺ CD45⁺) and a negative cell line FRN14.33 (CD14⁻ CD45⁻) were mixed in different proportions and a constant final number of cells, so that the positive line/negative line ratio of the mixture ranged from 0 to 100%.

In order to test the linearity of staining of CD16 specificity, whole blood (CD16⁺ granulocytes), and a negative FRN14.33 (CD16⁻) cell line were mixed in different proportions and with a constant final number of cells, so that the granulocytes/negative line ratio of the mixture ranged from 0 to 100%.

Aliquots were stained using the procedure described above and linear regression between the expected values and the observed values was calculated.

Specificity	Linear regression	Linearity (R ²)
CD14	Y = 0.974 X + 1.26	0.999
CD45	Y = 0.997 X + 0.49	0.999

Specificity	Linear regression	Linearity (R ²)
CD16	Y = 0.989 X + 0.46	0.999

EXPECTED VALUES

Each laboratory must compile a list of reference values based upon a group of healthy donors from the local population. This must be done by taking age, sex and ethnic group into account, as well as any other potential regional differences.

In our laboratories, the whole blood samples of 50 healthy adults were treated using the reagent described above.

The results obtained in the leucocyte sub-populations of interest in these 50 donors are shown in the tables below:

Lymphocytes	Number	Mean (%)	SD	CV (%)
CD16 ⁺	50	10.2	4.4	44

Monocytes	Number	Mean (%)	SD	CV (%)
CD14 ⁺	50	91.0	6.3	7
CD16 ⁺	50	350	12.6	36

Granulocytes	Number	Mean (%)	SD	CV (%)
CD14 ⁺	50	98.5	2.2	2.2
CD16 ⁺	50	90.2	9.3	10.3

INTRA-LABORATORY REPRODUCIBILITY

On the same day and using the same cytometer, 12 measurements of the percentage of staining of a positive target were carried out (monocytes and granulocytes from peripheral blood). The results obtained are summarized in the following table:

Monocytes	Number	Mean (%)	SD	CV (%)
CD14 ⁺	12	69	0.75	1.1

Granulocytes	Number	Mean (%)	SD	CV (%)
CD16 ⁺	12	98.1	0.16	0.16
CD45 ⁺	12	99.9	0.05	0.05

INTER-LABORATORY REPRODUCIBILITY

On the same day and on the same positive target (peripheral blood monocytes and granulocytes), 12 measurements of the percentage of stained cells were carried out by two technicians and the preparations analyzed using two different cytometers. The results obtained are summarized in the following tables:

Cytometer n° 1:

Monocytes	Number	Mean (%)	SD	CV (%)
CD14 ⁺	12	69	0.75	1.1

Granulocytes	Number	Mean (%)	SD	CV (%)
CD16 ⁺	12	98.1	0.16	0.16
CD45 ⁺	12	99.9	0.05	0.05

Cytometer n° 2:

Monocytes	Number	Mean (%)	SD	CV (%)
CD14 ⁺	12	74	0.35	0.9

Granulocytes	Number	Mean (%)	SD	CV (%)
CD16 ⁺	12	98.2	0.05	0.1
CD45 ⁺	12	99.8	0.05	0.05

LIMITATIONS OF THE TECHNIQUE

- Flow cytometry may produce false results if the cytometer has not been aligned perfectly, if fluorescence leaks have not been correctly compensated for and if the regions have not been carefully positioned.
- It is preferable to use a RBC lysis technique with a washing step as this reagent has not been optimized for "no wash" lysis techniques.
- Accurate and reproducible results will be obtained as long as the procedures used are in accordance with the technical insert leaflet and compatible with good laboratory practices.
- The conjugated antibodies of this reagent are calibrated so as to offer the best specific signal/non-specific signal ratio. Therefore, it is important to adhere to the reagent volume/sample volume ratio in every test.
- In the case of a hyperleucocytosis, dilute the blood in PBS so as to obtain a value of approximately 5 x 10⁹ leucocytes/L.
- In certain disease states, such as severe renal failure or haemoglobinopathies, lysis of red cells may be slow, incomplete or even impossible. In this case, it is recommended to isolate mononucleated cells using a density gradient (Ficoll, for example) prior to staining.
- CD45-negative or very weakly-positive acute lymphoblastic leukaemia have been described. For these, the lymphocytic origin of the blast cells should be confirmed using other markers.

MISCELLANEOUS

See the Appendix for examples and references.

TRADEMARKS

The Beckman Coulter logo, COULTER, ECD, EPICS, EXPO, Flow-Set, IOTest, System II, and XL are the registered trademarks of Beckman Coulter Inc.

Texas Red is a registered trademark of Molecular Probes Inc.

MANUFACTURED BY:

IMMUNOTECH
a Beckman Coulter Company
130 avenue de Lattre de Tassigny
B.P. 177 – 13276 Marseille Cedex 9
France
Customer Services: (33) 4 91 17 27 27

www.beckmancoulter.com



APPENDIX TO REF A07715

EXAMPLES

Conjugated Antibodies (Ref. A07715). Lysis and fixation are with IOTest 3 Lysing Solution (Ref. A07799) and IOTest 3 Fixative Solution (Ref. A07800) respectively.

The diagrams below are biparametric representations (Side Scatter versus Fluorescence Intensity or Fluorescence Intensity versus Fluorescence Intensity) of an Acute Myeloblastic Leukemia specimen (AML-M5, Bone marrow aspirate). Region A (CD45 positive blasts cluster) defines the gating strategy used on this example. All acquired events are shown. Gated events are shown in dark in all histograms.

Acquisition is performed with a COULTER® EPICS® XL™ flow cytometer equipped with System II™ software and analysis is with EXPO™ Cytometer software (Ref. 6605434).

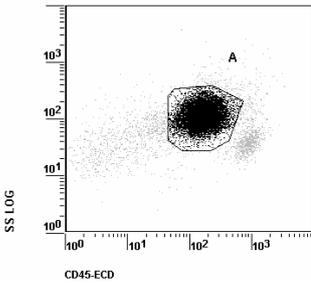


Figure 1

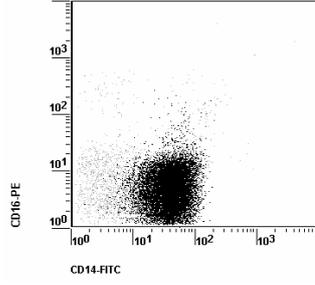


Figure 2

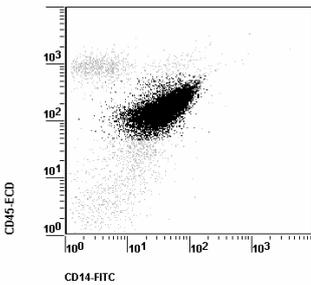


Figure 3

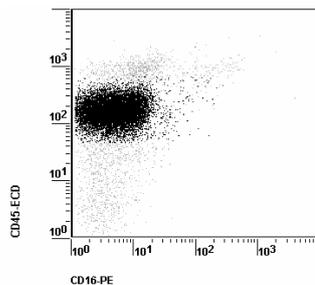


Figure 4

REFERENCES

1. Todd III, R.F., Nadler, L.M., Schlossman, S.F., "Antigens on human monocytes identified by monoclonal antibodies", 1981, *J. Immunol.*, 126, 1435-1442.
2. Ravetch, J.V., Perussia, B., "Alternative membrane forms of FcγRIII (CD16) on human natural killer cells and neutrophils", 1989, *J. Exp. Med.*, 170, 481-497.
3. Huizinga, T.W.J., Roos, D., Von dem Borne, A.E.G. Kr., "Neutrophil Fcγ receptors: A two-way bridge in the immune system", 1990, *Blood*, 75, 1211-1214.
4. Borowitz, M.J., Guenther, K.L., Shults, K.E., Stelzer, G.T., "Immunophenotyping of acute leukemia by flow cytometric analysis. Use of CD45 and right-angle light scatter to gate on leukemic blasts in three-color analysis", 1993, *Am. J. Clin. Pathol.*, 5, 100, 534-540.
5. Seltzer, G.T., Shults, K.E., Loken, M.R., "CD45 gating for routine flow cytometric analysis of human bone marrow specimens", 1993, *Acad. Sciences*, 265-280.
6. Ziegler-Heitbrock, H.W.L., Ulevitch, R.J., "CD14: Cell surface receptor and differentiation markers", 1993, *Immunol. Today*, 14, 121-125.
7. Goyert, S.M., Cohen, L., Gangloff, S.C., Ashmun, R., Haeflner-Cavaillon, N., "CD14 Workshop panel report", 1997, *Leucocyte Typing VI, White Cell Differentiation Antigens*. Kishimoto, T., et al, Eds., Garland Publishing, Inc., 963-965.
8. Schmidt, R.E., Perussia, B., "Cluster report: CD16", 1989, *Leucocyte Typing IV, White Cell Differentiation Antigens*. W. Knapp, et al., Eds., Oxford University Press, 574-578.
9. Cobbold, S., Hale, G., Waldmann, H., "Non-lineage, LFA-1 family, and leukocyte common antigens: New and previously defined clusters", 1987, *Leucocyte Typing III, White Cell Differentiation Antigens*, McMichael A.J., et al., Eds., Oxford University Press, 788-803.